




102 104 106 108 110

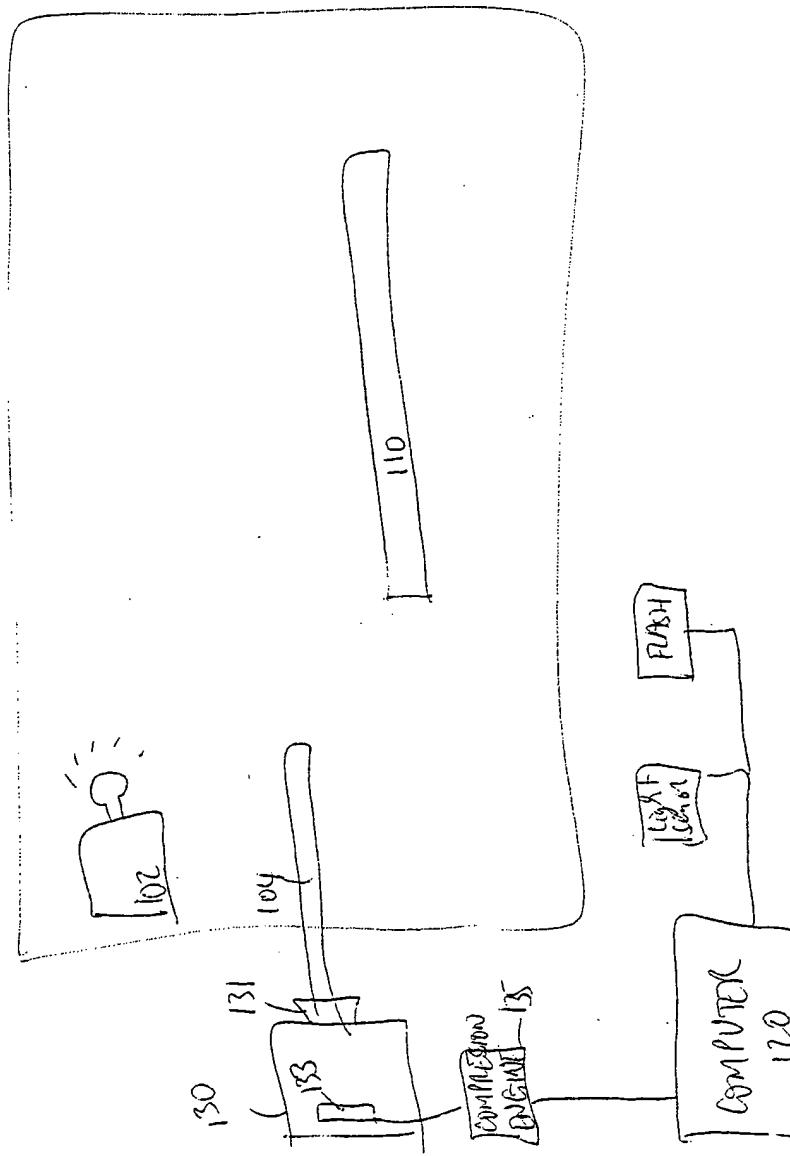

F1 G1

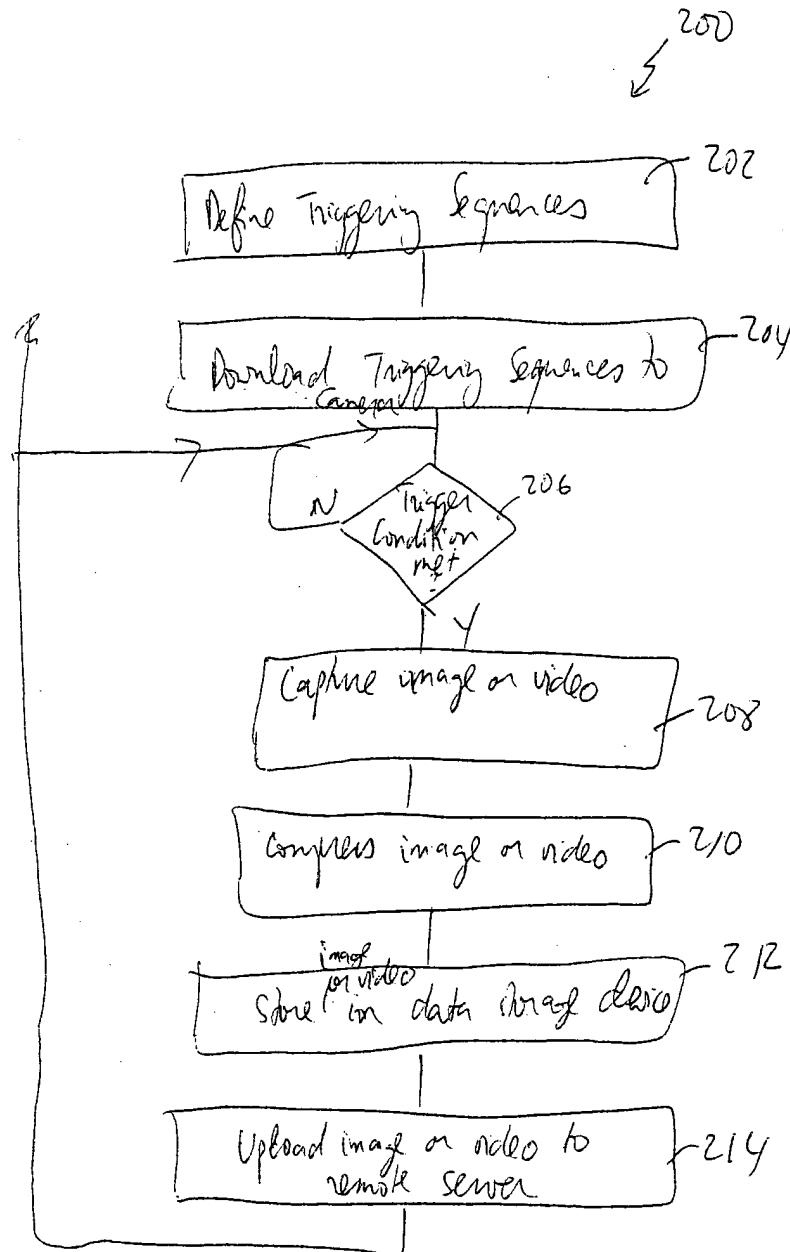

F. 2

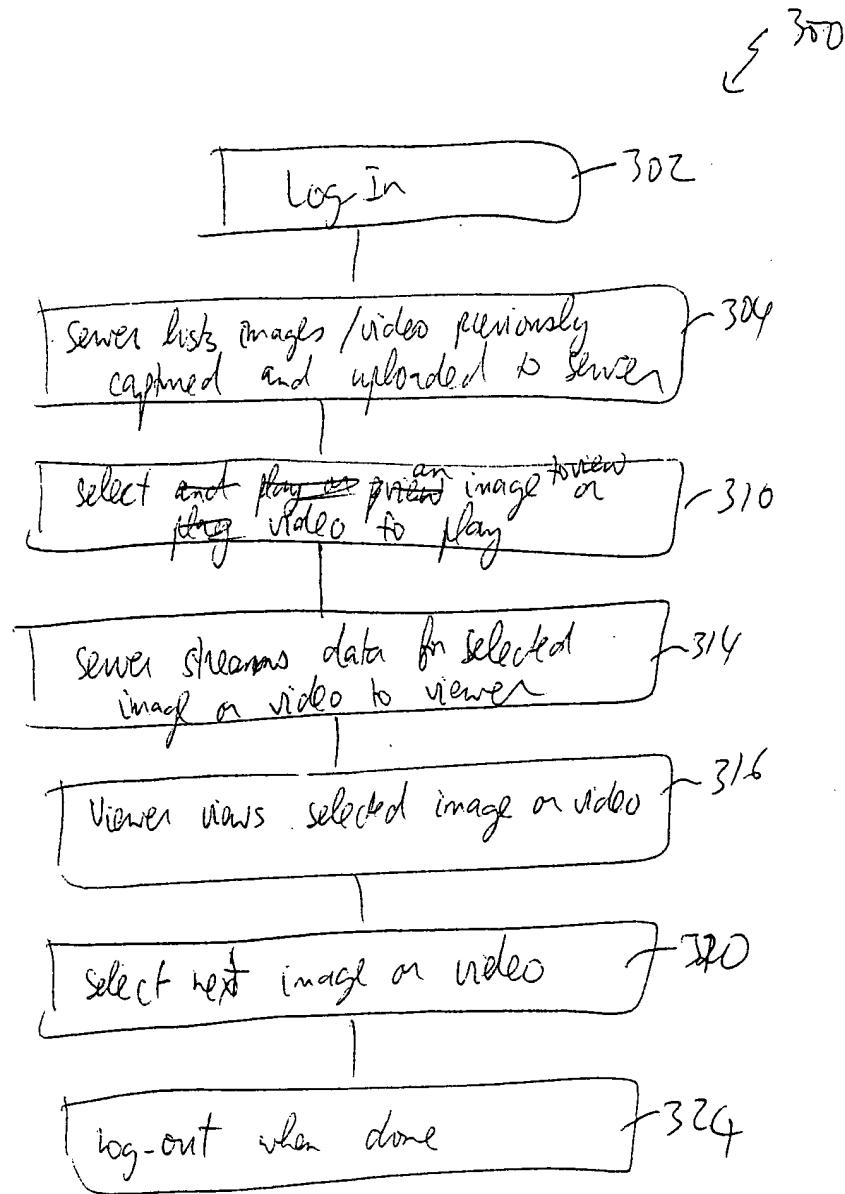

F. 3

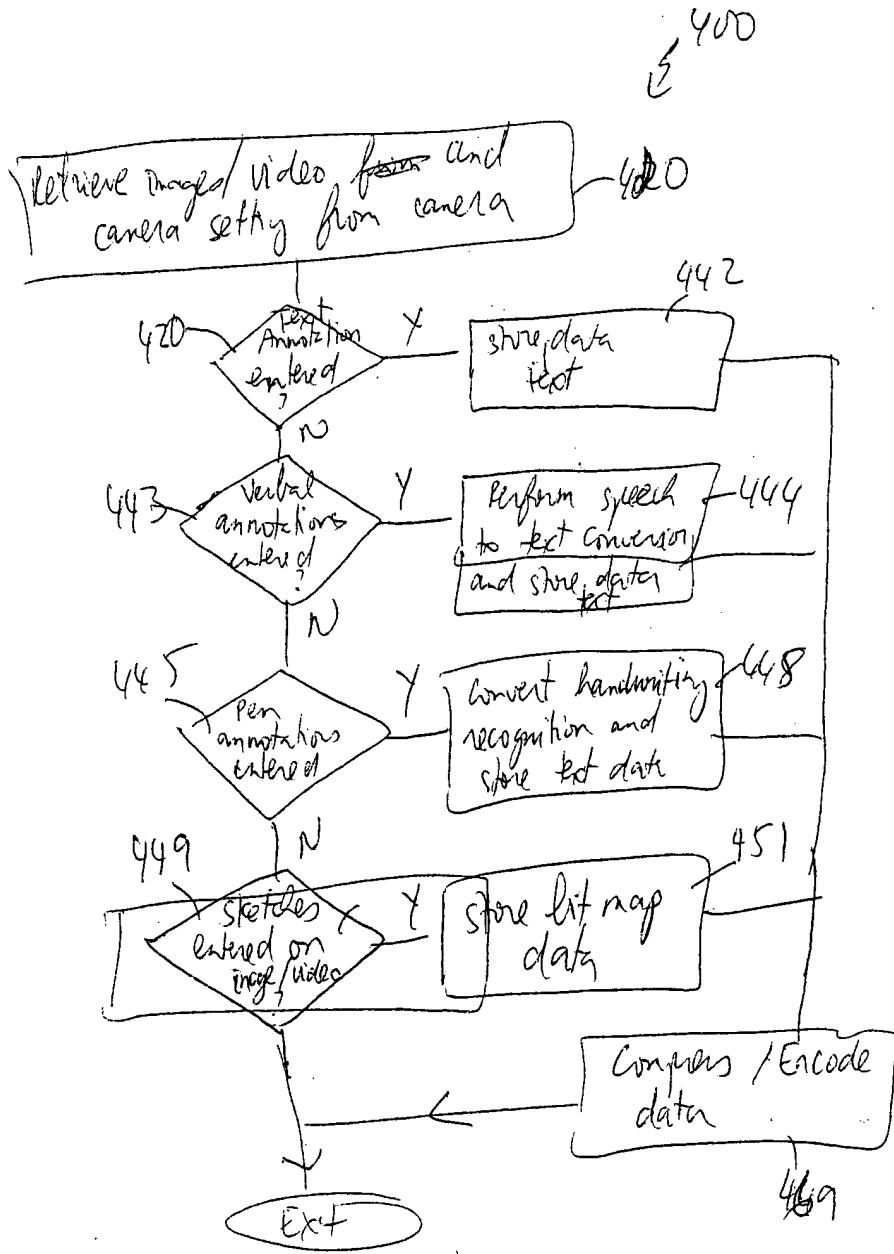


Fig. 4

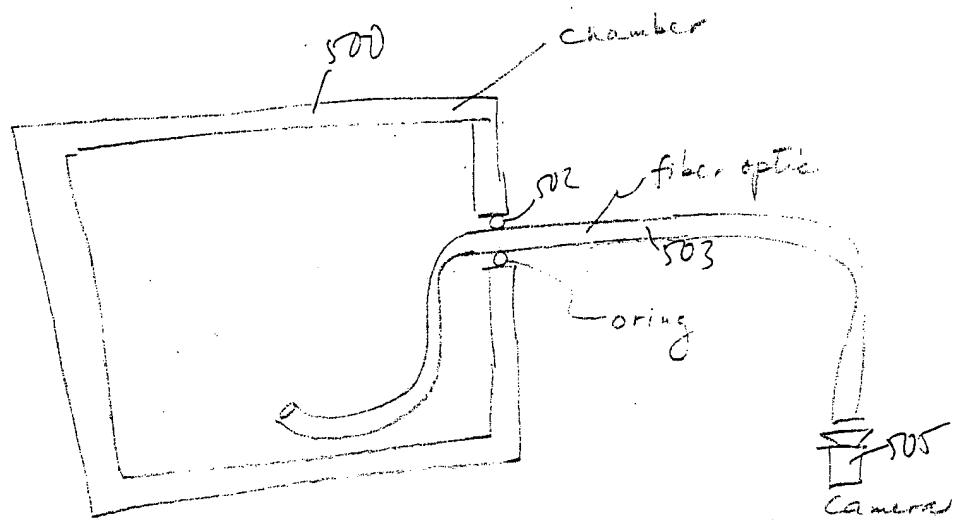


Fig 5
Vacuum adapter for viewing inside the
chamber

09/26/93 Schematic October 30th

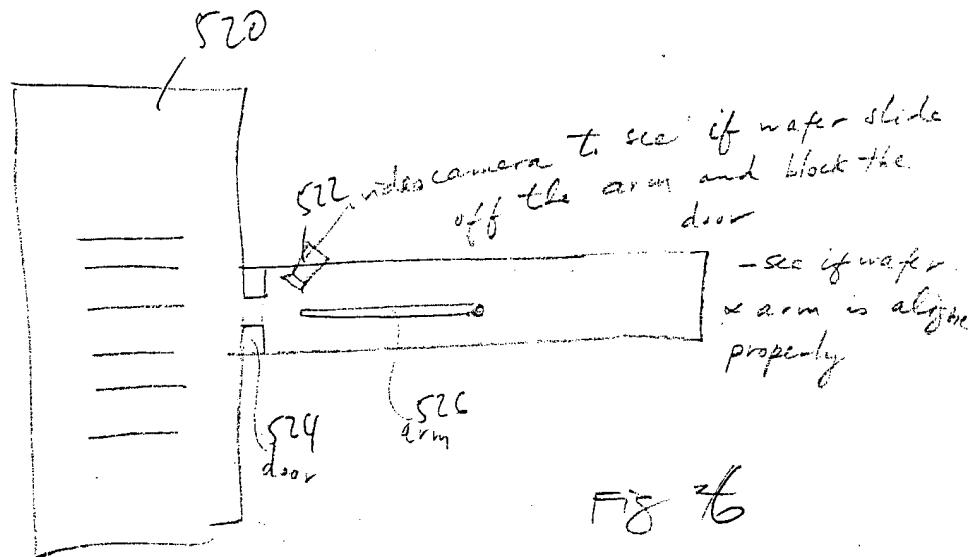


Fig 26

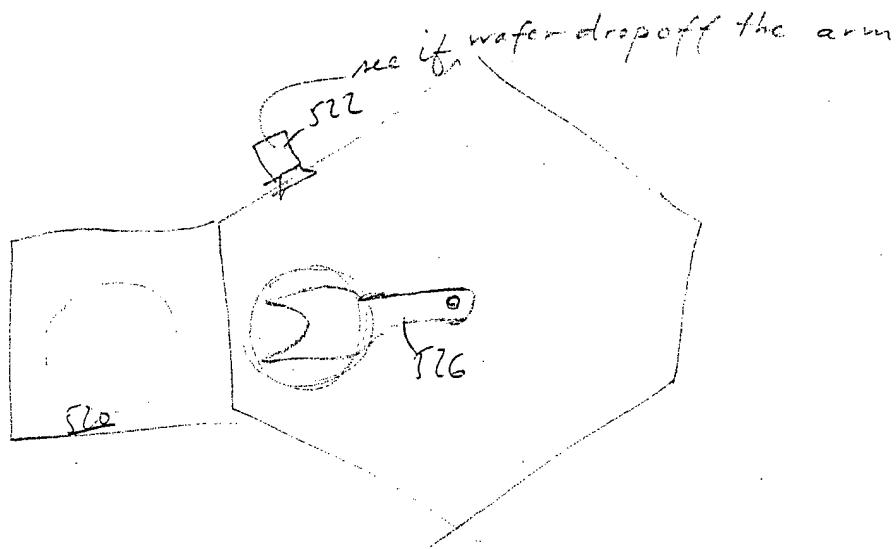


Fig 27

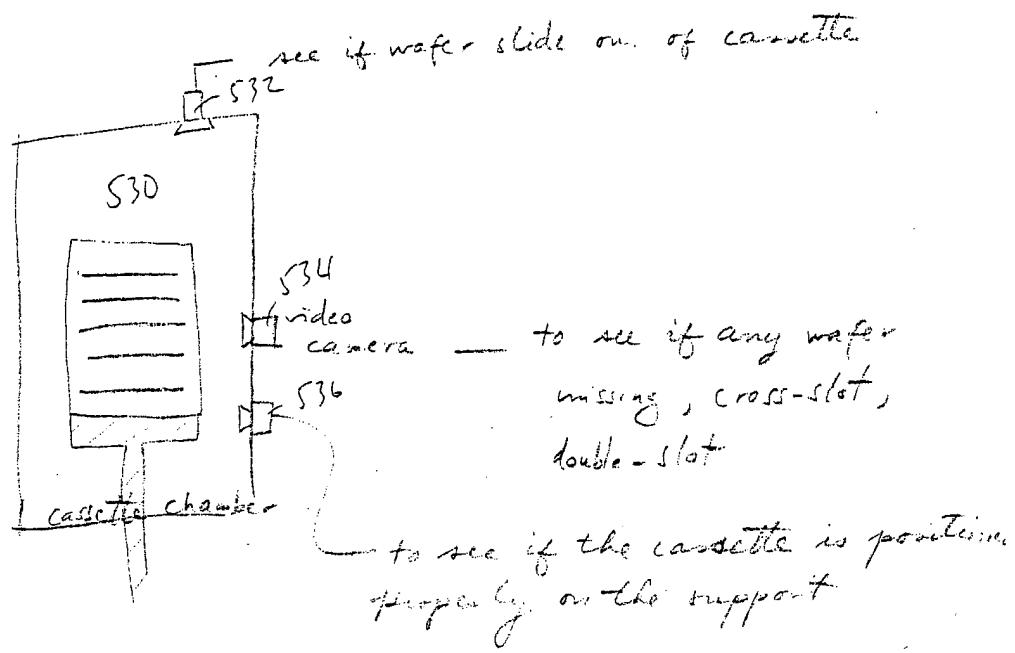


Fig 8

03765921 - 042301

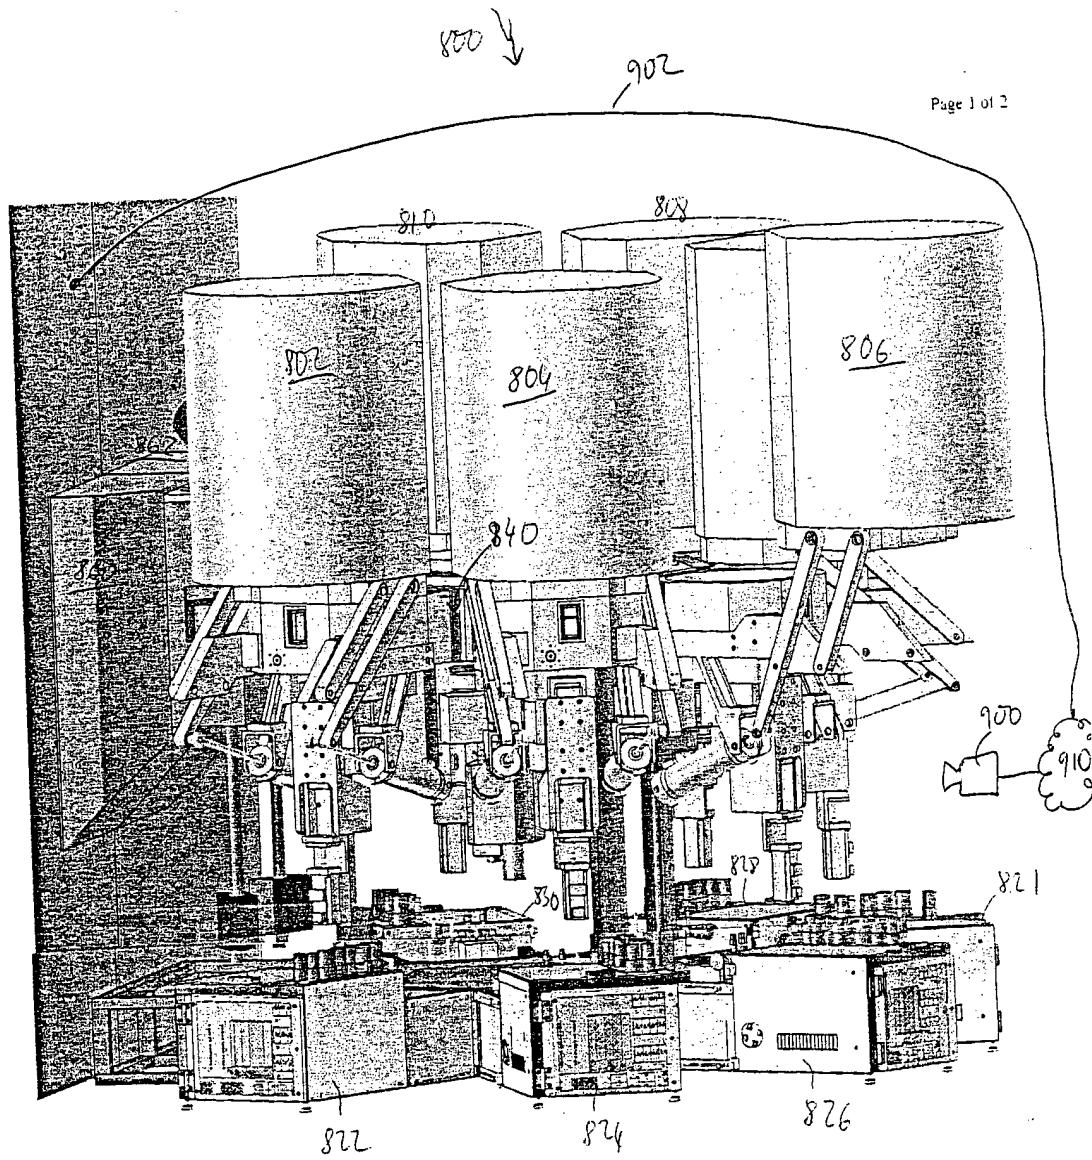


FIG. 9